

DEVITA BRT

BIORESONANCE TELEMETRIC CORECTION

DIGITAL DEVICE FOR ENDOGENOUS BIORESONANCE CORRECTION OF THE BODY

MANAGE YOUR HEALTH

AUTOMATED PROFESSIONAL METODOLOGY FOR DOMESTIC USE



PERSONAL ADJUSTMENT OF THE BODY



ACTIVATION OF THE ADAPTION ABILITIES



QUICKER RECOVERY



DEVITA BRT

BIORESONANCE TELEMETRIC CORRECTION

MANAGE YOUR HEALTH

- REASONABLE DIMENSIONS AND WEIGHT

- RECHARGEABLE BUILT-IN BATTERIES

- UNLIMITED NUMBER OF USERS

- COMPATIBLE WITH SEVERAL PROGRAMS OF DEVITA RITM AND DEVITA ENERGY

- DURATION OF ONE SESSION IS 20 MINUTES





DEVITA BRT


BIORESONANCE TELEMETRIC CORRECTION

HOW IT WORKS

BIORESONANCE TELEMETRY (BRT) – it is improvement of health state utilizing own electromagnetic oscillations of the patient.

DEVITA BRT INVERSIVE MODE


recording, strengthening and turning upside-down the pathogenic electromagnetic oscillations of the body; creates neutralizing interaction of pathogenic and correcting oscillations and restores healthy physiological oscillations of the patient's organism.

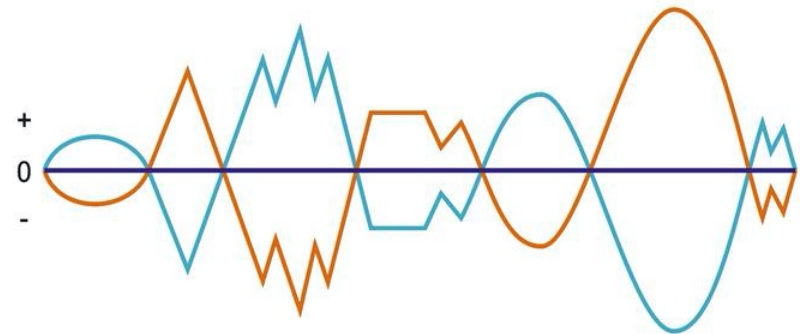

- Pathogenic oscillations
- Correcting oscillations (pathogenic oscillations inverted on 180°)
- Physiological oscillations



INVERSION (derives from the Latin word *Inversio* – turning over, upside-down) – the method invented by German Doctor Franz Morell and Engineer Erich Rasche in the middle of XX Century.

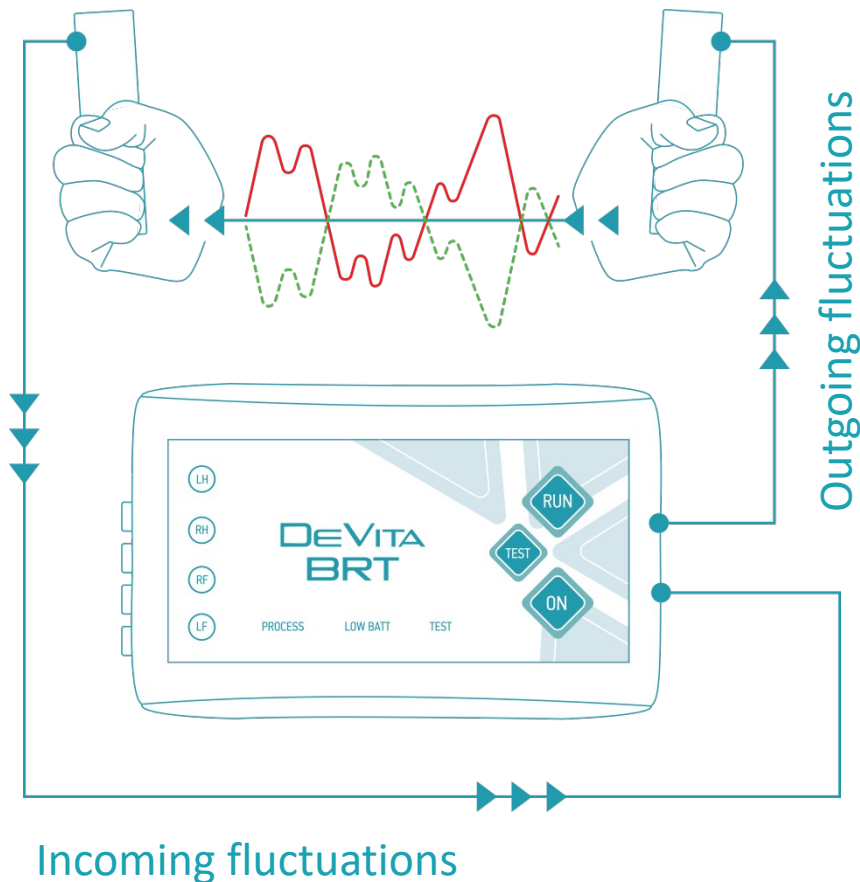REVERSE ACTIVATION (reverse order)



This process occurs during treatment with bioresonance. The purpose of the method is to destroy the abnormal electromagnetic oscillations present in the patient's body and so to achieve a state of improvement, which in turn enables complete restoration of the system.

Bioresonance therapy frees the body from interferences that prevent and block its energy.

-  Pathological fluctuations
-  Therapeutic fluctuations



Deta
Elis
Holding

BRT - LIMITS THE INFLAMMATION BY QUENCHING THE DISHARMONIC FREQUENCIES





DEVITA BRT

- It restores regularity in the mesenchyme (extracellular matrix, intracellular matrix, intranuclear matrix)
- It saves energy and balances the body, so as to strengthen its defense systems
- It limits the inflammation
- It disrupts pathogenic microorganisms
- It is an excellent symptomatic treatment in the acute phase of diseases
- It discharges the psychosomatic outbursts and charges
- It is decisive for smoking cessation and rehabilitation procedures



DEVITA BRT

BIORESONANCE TELEMETRIC CORRECTION

BIOLOGICAL FUNDAMENTALS OF INFLUENCE



EFFICIENTLY



SAFELY




PHYSIOLOGICALLY



CONVENIENTLY

Reading the electromagnetic oscillations of a person and health improving influence is implemented through the bio-active points of the body located within the zones of projection of the organs on the skin of arms and feet

SKETCH FOR THE DEVICE CONNECTION

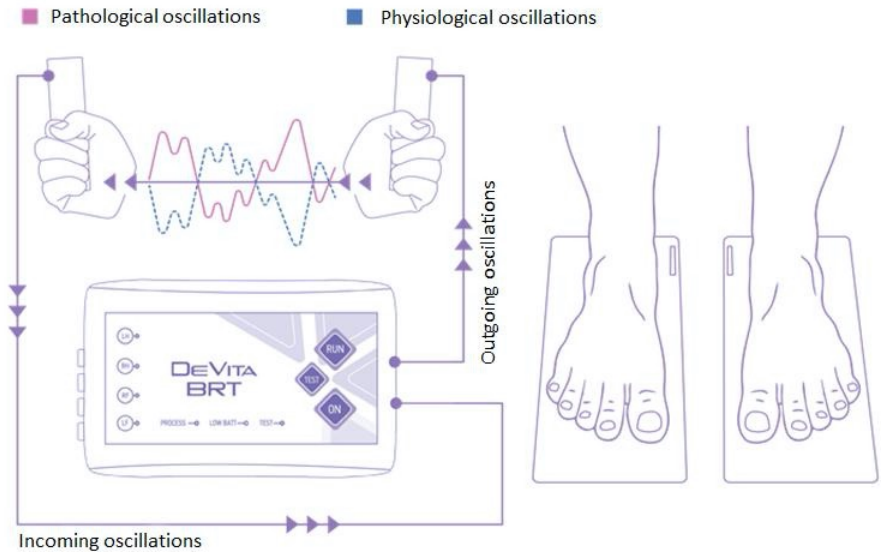

DEVITA BRT

BIORESONANCE TELEMETRIC CORRECTION

AUTOMATED PROFESSIONAL METHODOLOGY



EASY TO CONNECT



AUTOMATIC PROGRAM



EASY TO USE

STEP 1 Reads the own electromagnetic oscillations of the body.

STEP 2 Inverts and neutralizes pathogenic/disharmonious oscillations; strengthens physiological/harmonious oscillations.

STEP 3 Returns the physiological/harmonious oscillations to the human body.





DEVITA BRT

BIORESONANCE TELEMETRIC CORRECTION

THE NECESSARY CONDITIONS FOR AN EFFECTIVE HEALTH IMPROVING SESSION



24 HOURS BEFORE THE SESSION EXCLUDE SMOCKING, CONSUMPTION OF ALCOHOLIC BEVERAGES AND COFFEE



PRIOR THE SESSION IT IS RECOMMENDED TO IMPLEMENT ALL-ROUND ESTIMATION OF THE BODY STATE UTILIZING OUR DEPULS+ COMPLEX



THE SESSION LOCATION MUST NOT BE IN GEO-PATHOGENIC ZONE AND/OR HAVE ANY HARMFUL ELECTROMAGNETIC FIELDS



THE OPERATING ELECTRIC APPLIANCES MUST NOT BE CLOSER THAN 0.5 M FROM THE PLACE OF THE TREATMENT



USE THE CLOTHES MADE OF NATURAL FABRICS TO AVOID ACCUMULATION OF STATIC ELECTICITY



FOR BETTER CONTACT OF THE PALMS AND FEET WITH ELECTRODES PLEASE MOISTEN THE ELECTRODE SURFACE WITH A WET NAPKIN NOT CONTAINING ALCOHOL OR PERFUME

DEVITA BRT

BIORESONANCE TELEMETRIC CORRECTION

THE WAY OF COMBINED USE OF **DEVITA** DIGITAL DEVICES FOR PERFECT HEALTH IMPROVEMENT

DEVITA RITM MINI

Program:

- Active protection
- Anti-stress
- Blood circulation regulation
- Digestion
- Detoxification



DEVITA ENERGY MINI

Program:

- Energy

STEP 1 CHOOSE ON THE DIGITAL DEVICE **DEVITA RITM MINI** or **DEVITA ENERGY MINI** ONE OF THE SUGGESTED PROGRAMS

STEP 2 WHEN READY FOR THE BIORESONANCE TELEMETRIC CORRECTION SESSION TURN-ON ONE OF THE PROGRAMS YOU HAVE CHOSEN

NEVER USE BOTH **DEVITA RITM MINI** AND **DEVITA ENERGY MINI** DEVICES SIMULTANEOUSLY!