

DEVITA D

DEVITA D IS A DEVICE FOR COMPREHENSIVE HEALTH ASSESSMENT AND IMPROVEMENT



DEVITA D

A DEVICE FOR COMPREHENSIVE HEALTH ASSESSMENT AND IMPROVEMENT

WITH DEVITA D YOU CAN:



PERFORM A COMPREHENSIVE BODY ASSESSMENT;



DETECT THE PRESENCE OF VARIOUS TYPES OF ALLERGENS, TOXINS, PATHOGENIC MICROORGANISMS (VIRUSES, BACTERIA, PROTOZOA, FUNGI, AND HELMINTHS);



CONDUCT A DETAILED ASSESSMENT OF THE STATE OF SPECIFIC ORGANS AND SYSTEMS, TO SEE THE PRESENCE OF INFLAMMATORY PROCESSES;



IDENTIFY MICRO NUTRIENTS, ELEMENTS AND VITAMIN DEFICIENCIES IN THE BODY;



SELECT THE NECESSARY MEANS/METHODS TO MAINTAIN HEALTH;



SELECT HOMEOPATHIC REMEDIES, AND IDENTIFY THEIR COMPATIBILITY WHEN PRESCRIBING A COMPREHENSIVE RECOVERY REGIMEN;



CREATE AND MAINTAIN A CLIENT DATABASE;



WORK IN MANUAL AND AUTOMATIC MODES;



RECORD CUSTOM ELECTRONIC PREPARATIONS;




CREATE RECOMMENDATIONS WITH THE USE OF DEHOLDING PRODUCTS AND PROVIDE THEM TO THE CLIENT IN DIGITAL OR PRINTED FORM.

DEVITA D

A DEVICE FOR COMPREHENSIVE HEALTH ASSESSMENT AND IMPROVEMENT

DEVICE DESIGN

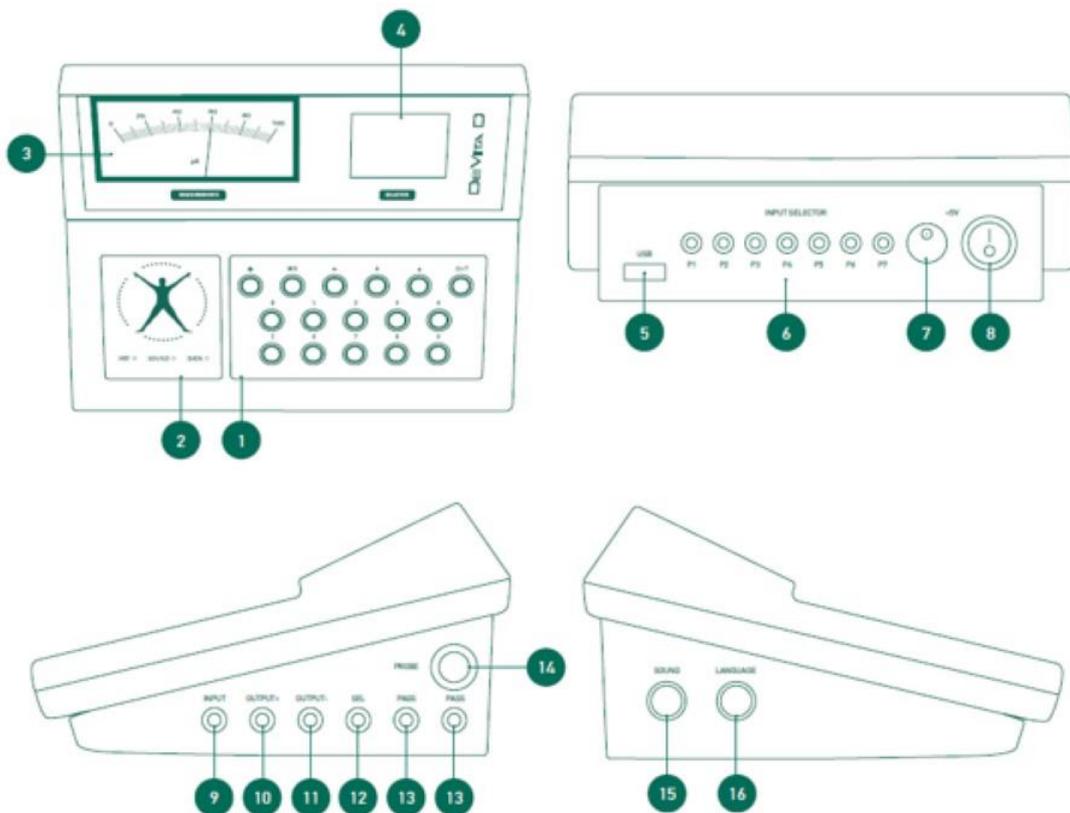

1. "SELECTOR" control panel
2. "MEASUREMENTS" control panel (testing)
3. Measuring instrument - display of the current measurement value
4. Display – display of preparation parameters
5. USB port – connection to computer
6. "P1-P7 INPUT SELECTOR" connectors – recording user (custom) preparations into the selector
7. "+5V" connector – external power supply connection
8. Power on/off switch
9. "INPUT" connector – reprinter (recording information) input
10. "OUTPUT+" connector – reprinter output for non-inverted preparations
11. "OUTPUT-" connector – reprinter output for inverted preparations
12. "SEL" connector – selector output, preparation dispensing
13. "PASS" connector – passive output of the device
14. "PROBE" connector – measuring probe connection
15. "SOUND" button – sound on/off
16. "LANGUAGE" button – language selection

DEVITA D

A DEVICE FOR COMPREHENSIVE HEALTH ASSESSMENT AND IMPROVEMENT

DEVICE CONNECTION



DEVITA D

A DEVICE FOR COMPREHENSIVE HEALTH ASSESSMENT AND IMPROVEMENT

WORKING WITH THE DEVICE. MEASURING UNIT

It is based on one of the most common electropuncture techniques, the method developed by Dr. R. Voll, which uses changes in the electrical resistance of the skin for testing.

THE UNIT INCLUDES:

1. Measuring scale in the range of 0-100 mA



MEASUREMENTS



2. Display buttons:

VRT – switching to VRT (Vegetative Resonance Test) mode

SOUND – switching on the sound

DATA – transfer of current measurements to the computer


DEVITA D

A DEVICE FOR COMPREHENSIVE HEALTH ASSESSMENT AND IMPROVEMENT

WORKING WITH THE DEVICE. SELECTOR UNIT

The selector contains 17,200 preparations for testing and recording homeopathic remedies. It allows for the recording of 18,200 custom preparations.

THE UNIT INCLUDES A KEYPAD AND A DISPLAY:

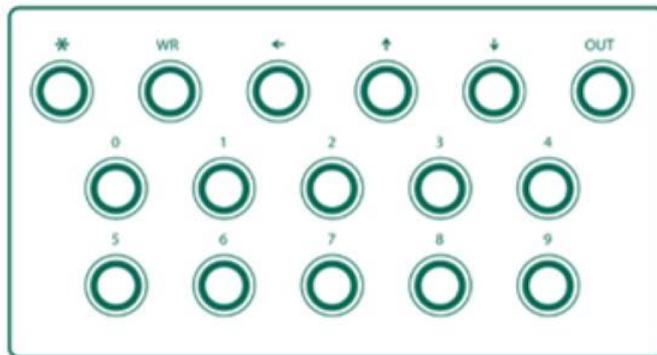

The keypad contains buttons:

- 0-9** – to enter the preparation number
- *** – to enter the preparation cell
- OUT** – to dispense the preparation
- ←** – to delete one or more preparations
- ↑ ↓** – to move through the list of selected preparations
- WR** – to record preparations



The display has windows:

- N** – level number (18 in total)
- Address** – preparation number
- Cell** – cell number
- EN** – display language
- information about the current preparation

DEVITA D

A DEVICE FOR COMPREHENSIVE HEALTH ASSESSMENT AND IMPROVEMENT

WORKING WITH THE DEVICE. SETTINGS



LANGUAGE SELECTION

Press the LANGUAGE button to select the desired language.

SOUND SETTING

If you press the SOUND button, you can perform tests with an audible signal sounding when you apply pressure on biologically active points (BAP).

DEVITA D

A DEVICE FOR COMPREHENSIVE HEALTH ASSESSMENT AND IMPROVEMENT

“ACTIVE REPRINTER” MODE

It is used to copy properties of original preparations to other media (water, sodium chloride solution, milk sugar, wax).

INPUT – socket to connect the cuvette stand or the honeycomb plate with selected original preparations.

OUTPUT+ – socket to connect the cuvette stand with a carrier substance for recording direct information.

OUTPUT- – socket to connect the cuvette stand with a carrier substance for recording inverted information.

CONNECTORS FOR TESTING

PROBE – socket for probe connection.

SEL – socket for dispensing of preparations.

PASS – socket to connect the passive electrode for testing.

The two **PASS** sockets are equivalent.



DEVITA D

A DEVICE FOR COMPREHENSIVE HEALTH ASSESSMENT AND IMPROVEMENT

RECORDING OF PREPARATIONS TO THE SELECTOR

The device can record 18,200 preparations.

Recording is performed simultaneously in 7 cells at the same address.



DEVITA D

A DEVICE FOR COMPREHENSIVE HEALTH ASSESSMENT AND IMPROVEMENT

BENEFITS OF DEVITA D

- Lightweight and compact;
- Highly accurate results (over 85% accuracy);
- Safe (even for children);
- Universal (for anyone and everyone);
- Effective (allows you to identify problems at the initial stages);
- Informative (helps answer basic questions: what, where, when);
- Contains over 17,000 preparations and has the ability to record over 18,000 preparations;
- Has the ability to correct the condition of the body.